

# Human IL-2 sR $\alpha$ ELISA Kit

For the quantitative determination of human interleukin-2 soluble receptor alpha (IL-2 sR $\alpha$ ) concentrations in serum, plasma, cell culture supernatant, and other biological fluids.

Catalogue Number: EL10033

*96 tests*

FOR LABORATORY RESEARCH USE ONLY.  
NOT FOR DIAGNOSTIC USE



**ANOGEN**

2355 Derry Road East, Unit 23  
Mississauga, Ontario  
CANADA L5S 1V6  
Tel: (905) 677-9221 or (877) 755-8324  
Fax: (905) 677-0023

Email: [info@anogen.ca](mailto:info@anogen.ca) ♦ Web Site: [www.anogen.ca](http://www.anogen.ca)

## TABLE OF CONTENTS

	Page
INTENDED USE	2
INTRODUCTION	2
PRINCIPLE OF THE ASSAY	3
LIMITATIONS OF APPLICATION	3
REAGENTS PROVIDED	4
MATERIALS REQUIRED BUT NOT SUPPLIED	5
PRECAUTIONS	5
SAMPLE PREPARATION	6
.....Collection, Handling and Storage	6
PREPARATION OF REAGENTS	6
ASSAY PROCEDURE	8
CALCULATION OF RESULTS	9
TYPICAL DATA	9
.....Example one (Calibrator Diluent I)	10
.....Example two (Calibrator Diluent II)	10
PERFORMANCE CHARACTERISTICS	11
.....Intra-assay precision	11
.....Inter-assay precision	12
.....Recovery	12
.....Sensitivity	12
.....Specificity	12
.....Expected Normal Values	13
REFERENCES	13

## INTENDED USE

This Human Interleukin-2 soluble receptor alpha ELISA Kit is to be used for the *in vitro* quantitative determination of human interleukin-2 soluble receptor alpha (IL-2 sR $\alpha$ ) concentrations in serum, plasma, cell culture supernatant, and other biological fluids. This kit is intended FOR LABORATORY RESEARCH USE ONLY and is not to be used in diagnostic or therapeutic procedures.

## INTRODUCTION

The biological function of IL-2 is obtained by binding to the specific interleukin-2 receptor (IL-2R). The IL-2R consists of three non-covalently linked chains, all of which are type I transmembrane proteins and include the  $\alpha$  chain (IL-2R $\alpha$ , p55),  $\beta$  chain (IL-2R $\beta$ , p75), and  $\gamma$  chain (IL-2R $\gamma$ , p65). The  $\alpha$  chain is cleaved from the cell surface via nonspecific proteolysis.

IL-2R $\alpha$  and IL-2R $\beta\gamma$  dimers bind to different residues on the IL-2 protein. The IL-2R $\alpha$  complex displays low affinity and the IL-2R $\alpha\beta$  complex displays intermediate affinity for IL-2 binding. Both IL-2R $\alpha$  and IL-2R $\alpha\beta$  complexes are unable to transduce a signal. The IL-2R $\beta\gamma$  complex has intermediate affinity for IL-2 binding and can transduce a signal with a relatively high concentration of IL-2. The IL-2R $\alpha\beta\gamma$  trimer is the high-affinity receptor for IL-2 and can transduce a signal successfully.

Many cells are capable of expressing IL-2R $\alpha$  including the antigen-activated T cells and B cells, and approximately 10% of natural killer (NK) cells, leukemia and lymphoma cells. When produced by activated T cells, the  $\alpha$  chain is 10-20 folds in excess of the  $\beta$  and  $\gamma$  chain. A soluble IL-2R $\alpha$  can be detected in tissue culture media of IL-2R $^+$  cells and in the serum of experimental animals and humans undergoing an immune response.

The major biological activities of IL-2R include promoting the proliferative expansion of T cells and NK cells upon activation, promoting the persistence of antigen-selected memory T cells, and promoting homeostasis of the immune system after it has successfully responded to an antigen. However, the biological activity of soluble IL-2R $\alpha$  is unclear. It has been reported that elevated IL-2 sR $\alpha$  level is accompanied by increased T and B cell activation and immune system activation as observed in rheumatoid arthritis, systemic lupus erythematosus (SLE), some leukemias and lymphomas. Because of its low affinity, IL-2 sR $\alpha$  would be expected to be an inhibitor of IL-2.

*This IL-2 sR $\alpha$  ELISA is a ready-to-use 4.5-hour solid phase immunoassay capable of measuring IL-2 sR $\alpha$  levels in serum, plasma, cell culture supernatant, and other biological fluids in the range of 0 to 2000 pg/mL. This assay has shown no cross-reactivity with other cytokines tested, and is expected to be used effectively for further investigations into the relationship between IL-2 sR $\alpha$  and the various conditions mentioned.*

## **PRINCIPLE OF THE ASSAY**

This IL-2 sR $\alpha$  enzyme linked immunosorbent assay (ELISA) applies a technique called a quantitative sandwich immunoassay. The microtiter plate provided in this kit has been pre-coated with a monoclonal antibody specific to IL-2 sR $\alpha$ . Standards or samples are then added to the appropriate microtiter plate wells with a biotin-conjugated polyclonal antibody preparation specific for IL-2 sR $\alpha$  and incubated. IL-2 sR $\alpha$  if present, will bind and become immobilized by the antibody pre-coated on the wells and then become “sandwiched” by biotin conjugate. The microtiter plate wells are thoroughly washed to remove unbound IL-2 sR $\alpha$  and other components of the sample. In order to quantitatively determine the amount of IL-2sR $\alpha$  present in the sample, Avidin conjugated to Horseradish Peroxidase (HRP) is added to each microplate well and incubated. Avidin is a tetramer containing four identical subunits, each having a high affinity-binding site for biotin. The wells are thoroughly washed to remove all unbound HRP-conjugated Avidin and a TMB (3,3',5, 5' tetramethyl-benzidine) substrate solution is added to each well. The enzyme (HRP) and substrate are allowed to react over a short incubation period. Only those wells that contain IL-2 sR $\alpha$ , biotin-conjugated antibody, and enzyme-conjugated Avidin will exhibit a change in colour. The enzyme-substrate reaction is terminated by the addition of a sulphuric acid solution and the colour change is measured spectrophotometrically at a wavelength of 450nm  $\pm$  2nm.

In order to measure the concentration of IL-2 sR $\alpha$  in the samples this kit includes two calibration diluents (Calibrator Diluent I for serum/plasma testing and Calibrator Diluent II for cell culture supernatant testing.) According to the testing system, the provided standard is diluted (2-fold) with the appropriate Calibrator Diluent and assayed at the same time as the samples. This allows the operator to produce a standard curve of Optical Density (O.D) versus IL-2 sR $\alpha$  concentration (pg/mL). The concentration of IL-2 sR $\alpha$  in the samples is then determined by comparing the O.D. of the samples to the standard curve.

## **LIMITATIONS OF APPLICATION**

- This Human IL-2 sR $\alpha$  ELISA kit is for laboratory research use only, and is not intended for use in clinical diagnostic procedures.
- Although all manufacturing precautions have been exercised to ensure that this product will be suitable for use with all validated sample types as designated in the product insert, the possibility of interference cannot be excluded due to the variety of proteins that may exist within the sample.
- The Calibrator Diluent selected for the standard curve should be consistent with the assay samples. If the values generated by the samples are greater than the uppermost standard, the samples dilution should be adjusted with the appropriate Calibrator Diluent and the assay should be repeated.

## REAGENTS PROVIDED

All reagents provided are stored at 2-8°C. Refer to the expiration date on the label.

		<b>96 tests</b>
1.	<b>IL-2 sR<math>\alpha</math> MICROTITER PLATE</b> (Part EL33-1) _____ Pre-coated with anti-human IL-2 sR $\alpha$ monoclonal antibody.	<b>96 wells</b>
2.	<b>BIOTIN CONJUGATE</b> (Part EL33-2) _____ Anti-human IL-2 sR $\alpha$ polyclonal antibody conjugated to Biotin.	<b>7 mL</b>
3.	<b>AVIDIN CONJUGATE</b> (Part EL33-3) _____ Avidin conjugated to horseradish peroxidase.	<b>12 mL</b>
4.	<b>IL-2 sR<math>\alpha</math> STANDARD</b> (Part EL33-4) _____ Recombinant human IL-2 sR $\alpha$ (4000 pg/vial) in a buffered protein base with preservative, lyophilized.	<b>2 vials</b>
5.	<b>CALIBRATOR DILUENT I</b> (EL33-5) _____ Animal serum with buffer and preservative. <i>For serum/plasma testing.</i>	<b>25 mL</b>
6.	<b>CALIBRATOR DILUENT II</b> (EL33-6) _____ Cell culture medium with calf serum and preservative. <i>For cell culture supernatant testing.</i>	<b>25 mL</b>
7.	<b>WASH BUFFER (20X)</b> (Part 30005) _____ 20-fold concentrated solution of buffered surfactant.	<b>60 mL</b>
8.	<b>SUBSTRATE A</b> (Part EL33-7) _____ Buffered solution with H <sub>2</sub> O <sub>2</sub>	<b>10 mL</b>
9.	<b>SUBSTRATE B</b> (Part 30007) _____ Buffered solution with TMB.	<b>10 mL</b>
10.	<b>STOP SOLUTION</b> (Part 30008) _____ 2N Sulphuric Acid (H <sub>2</sub> SO <sub>4</sub> ). Caution: Caustic Material!	<b>14 mL</b>

## MATERIALS REQUIRED BUT NOT SUPPLIED

1. Single or multi-channel precision pipettes with disposable tips: 10-100 $\mu$ L and 50-200 $\mu$ L for running the assay.
2. Pipettes: 1 mL, 5 mL, 10 mL, and 25 mL for reagent preparation.
3. Multi-channel pipette reservoir or equivalent reagent container.
4. Test tubes and racks.
5. Polypropylene tubes or containers (25 mL).
6. Erlenmeyer flasks: 100 mL, 400 mL, 1 L and 2 L.
7. Microtiter plate reader (450 nm  $\pm$  2nm).
8. Automatic microtiter plate washer or squirt bottle.
9. Sodium hypochlorite solution, 5.25% (household liquid bleach).
10. Deionized or distilled water.
11. Plastic plate cover.
12. Disposable gloves.
13. Absorbent paper.

## PRECAUTIONS

1. Do not substitute reagents from one kit lot to another. Standard, conjugate and microtiter plates are matched for optimal performance. Use only the reagents supplied by manufacturer.
2. Allow kit reagents and materials to reach room temperature (20-25°C) before use. Do not use water baths to thaw samples or reagents.
3. Do not use kit components beyond their expiration date.
4. Use only deionized or distilled water to dilute reagents.
5. Do not remove microtiter plate from the storage bag until needed. Unused strips should be stored at 2-8°C in their pouch with the desiccant provided.
6. Use fresh disposable pipette tips for each transfer to avoid contamination.
7. Do not mix acid and sodium hypochlorite solutions.
8. Human serum and plasma should be handled as potentially hazardous and capable of transmitting disease. Disposable gloves must be worn during the assay procedure since no known test method can offer complete assurance that products derived from human blood will not transmit infectious agents. Therefore, all blood derivatives should be considered potentially infectious and good laboratory practices should be followed.
9. All samples should be disposed of in a manner that will inactivate human viruses.  
Solid Waste: Autoclave 60 min. at 121°C.  
Liquid Waste: Add sodium hypochlorite to a final concentration of 1.0%. The waste should be allowed to stand for a minimum of 30 minutes to inactivate the viruses before disposal.
10. Substrate Solution is easily contaminated. If bluish prior to use, *do not use*.
11. Substrate B contains 20% acetone, keep this reagent away from sources of heat or flame.
12. If Wash Buffer (20X) is stored at a lower temperature (2-5°C), crystals may form which must be dissolved by warming to 37°C prior to use.

## SAMPLE PREPARATION

### COLLECTION, HANDLING AND STORAGE

- a) **Cell Culture Supernatant:** Centrifuge to remove any visible particulate material.
- b) **Serum:** Blood should be drawn using standard venipuncture techniques and serum separated from the blood cells as soon as possible. Samples should be allowed to clot for one hour at room temperature, centrifuged for 10 minutes (4°C) and serum extracted.
- c) **Plasma:** Blood should be drawn using standard venipuncture techniques and plasma collected using sodium citrate, EDTA, or heparin as an anticoagulant. To ensure optimal recovery and minimal platelet contamination, after collection there must be quick separation of plasma with less than 30 minutes on ice. Centrifuge for 10 minutes (4°C) to remove any particulates. *This IL-2 sR $\alpha$  ELISA kit is not affected by haemolysis of specimens. No adverse effects have been noted in the presence of anti-coagulants, sodium citrate, EDTA, or heparin.*
  - Avoid grossly hemolytic, lipidic or turbid samples.
  - Serum, plasma, and cell culture supernatant samples to be used within 24-48 hours may be stored at 2-8°C, otherwise samples must stored at -20°C to avoid loss of bioactivity and contamination. Avoid freeze-thaw cycles.
  - When performing the assay slowly bring samples to room temperature.
  - It is recommended that all samples be assayed in duplicate.
  - DO NOT USE HEAT-TREATED SPECIMENS.

## PREPARATION OF REAGENTS

Remove all kit reagents from refrigerator and allow them to reach room temperature (20-25°C). Prepare the following reagents as indicated below. Mix thoroughly by gently swirling before pipetting. Avoid foaming.


1. **Wash Buffer (1X):** Add 60 mL of Wash Buffer (20X) and dilute to a final volume of 1200 mL with distilled or deionized water. Mix thoroughly. If a smaller volume of Wash Buffer (1X) is desired, add 1 volume of Wash Buffer (20X) to 19 volumes of distilled or deionized water. Wash Buffer (1X) is stable for 1 month at 2-8°C. Mix well before use.
2. **Substrate Solution:** Substrate A and Substrate B should be mixed together in equal volumes up to 15 minutes before use. Refer to the table provided for correct amounts of Substrate Solution to prepare.

Strips Used	Substrate A (mL)	Substrate B (mL)	Substrate Solution (mL)
2 strips (16 wells)	2.0	2.0	4.0

4 strips (32 wells)	3.0	3.0	6.0
6 strips (48 wells)	4.0	4.0	8.0
8 strips (64 wells)	5.0	5.0	10.0
10 strips (80 wells)	6.0	6.0	12.0
12 strips (96 wells)	7.0	7.0	14.0

3. **IL-2 sR $\alpha$  Standard:**

- a) Two vials of Standard are provided in this kit to allow both serum/plasma and cell culture supernatant testing. Reconstitute IL-2 sR $\alpha$  Standard with 2.0 mL of Calibrator Diluent I or Calibrator Diluent II. This reconstitution produces a stock solution of 2000 pg/mL. Allow solution to sit for at least 15 minutes with gentle agitation prior to making dilutions. Use within one hour of reconstituting. The IL-2 sR $\alpha$  standard stock solution can be stored frozen (-20°C) for up to 30 days. Avoid freeze-thaw cycles. Aliquot if repeated use is expected.
- b) Use the above stock solution to produce a serial 2-fold dilution series, as described below, within the range of this assay (62.5 to 2000 pg/mL) as illustrated. Add 0.5 mL of the appropriate Calibrator Diluent to each test tube. Between each test tube transfer be sure to mix contents thoroughly. The undiluted IL-2 sR $\alpha$  stock solution will serve as the high standard (2000 pg/mL) and the Calibrator Diluent will serve as the zero standard (0 pg/mL).

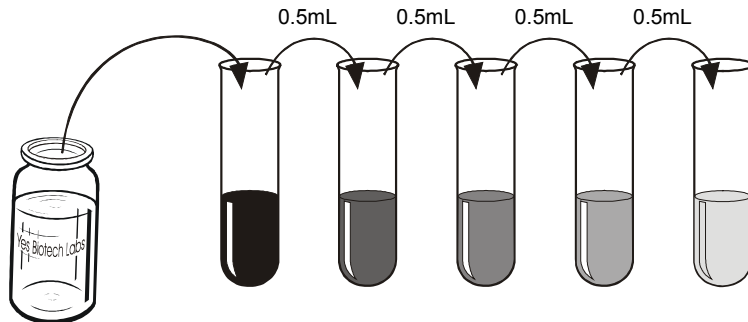

IL-2 sR $\alpha$ Standard	1000 pg/ml	500 pg/ml	250pg/ml	125 pg/ml	62.5 pg/ml
	2000 pg/ml				

## ASSAY PROCEDURE

1. Prepare Wash Buffer and IL-2 sR $\alpha$  Standards before starting assay procedure (see Preparation of Reagents). *It is recommended that the table and diagram provided be used as a reference for adding Standards and Samples to the Microtiter Plate.*

Wells	Contents	Wells	Contents
<b>1A, 1B</b>	Standard 1 <b>0 pg/mL</b> (S1)	<b>2A, 2B</b>	Standard 5 <b>500 pg/mL</b> (S6)
<b>1C, 1D</b>	Standard 2 <b>62.5 pg/mL</b> (S2)	<b>2C, 2D</b>	Standard 6 <b>1000 pg/mL</b> (S7)
<b>1E, 1F</b>	Standard 3 <b>125 pg/mL</b> (S3)	<b>2E, 2F</b>	Standard 7 <b>2000 pg/mL</b> (S7)
<b>1G, 1H</b>	Standard 4 <b>250 pg/mL</b> (S4)	<b>2G, 2H</b>	<b>IL-2 sR<math>\alpha</math> samples</b>

	1	2	3	4	5	6	7	8	9	10	11	12
<b>A</b>	S1	S5	2	6	10	14	18	22	26	30	34	38
<b>B</b>	S1	S5	2	6	10	14	18	22	26	30	34	38
<b>C</b>	S2	S6	3	7	11	15	19	23	27	31	35	39
<b>D</b>	S2	S6	3	7	11	15	19	23	27	31	35	39
<b>E</b>	S3	S7	4	8	12	16	20	24	28	32	36	40
<b>F</b>	S3	S7	4	8	12	16	20	24	28	32	36	40
<b>G</b>	S4	1	5	9	13	17	21	25	29	33	37	41
<b>H</b>	S4	1	5	9	13	17	21	25	29	33	37	41

2. Add 100 $\mu$ L of Standard or Sample to the appropriate well of the antibody pre-coated Microtiter Plate and incubate 1 hour at room temperature.
3. Without discarding the standards and samples, add 50 $\mu$ L Anti- IL-2 sR $\alpha$  Biotin conjugate to each wells. Mix well. Cover and incubate for 1 hour at room temperature.
4. Wash the Microtiter Plate using one of the specified methods indicated below:

Manual Washing: Remove incubation mixture by aspirating contents of the plate into a sink or proper waste container. Using a squirt bottle, fill each well completely with Wash Buffer (1X) then aspirate contents of the plate into a sink or proper waste container. Repeat this procedure four more times for a **total of FIVE washes**. After final wash, invert plate, and blot dry by hitting plate onto absorbent paper or paper towels until no moisture appears. *Note:* Hold the sides of the plate frame firmly when washing the plate to assure that all strips remain securely in frame.

Automated Washing: Aspirate all wells, then wash plates **FIVE times** using Wash Buffer (1X). Always adjust your washer to aspirate as much liquid as possible and set fill volume at 350  $\mu$ L/well/wash (range: 350-400  $\mu$ L). After final wash, invert plate, and blot dry by hitting plate onto absorbent paper or paper towels until no moisture appears. *It is recommended that the washer be set for a soaking time of 10 seconds or shaking time of 5 seconds between washes.*

5. Dispense 100 $\mu$ l of Avidin Conjugate to each well Mix well. Cover and incubate for 1 hour at room temperature.
6. Prepare Substrate Solution no more than 15 minutes before end of second incubation (see Preparation of Reagents).
7. Repeat wash procedure as described in Step 4.
8. Add 100 $\mu$ L Substrate Solution to each well. Cover and incubate for 15 minutes at room temperature.
9. Add 100 $\mu$ L Stop Solution to each well. Mix well.
10. Read the Optical Density (O.D.) at 450 nm using a microtiter plate reader set within 30 minutes.

## CALCULATION OF RESULTS

The standard curve is used to determine the amount of IL-2 sR $\alpha$  in an unknown sample. The standard curve is generated by plotting the average O.D. (450 nm) obtained for each of the standard concentrations on the vertical (Y) axis versus the corresponding IL-2 sR $\alpha$  concentration (pg/mL) on the horizontal (X) axis.

1. First, calculate the mean O.D value for each standard and sample. All O.D. values are subtracted by the value of the zero standard (0 pg/mL) before result interpretation. Construct the standard curve using graph paper or statistical software.
2. To determine the amount of IL-2 sR $\alpha$  in each sample, first locate the O.D. value on the Y-axis and extend a horizontal line to the standard curve. At the point of intersection, draw a vertical line to the X-axis and read the corresponding IL-2 sR $\alpha$  concentration. If samples generate values higher than the highest standard, dilute the samples and repeat the assay, the concentration read from the standard curve must be multiplied by the dilution factor.


## TYPICAL DATA

Results of a typical standard run of an IL-2 sR $\alpha$  ELISA are shown below. Any variation in standard diluent, operator, pipetting and washing technique, incubation time or temperature, and kit age can cause variation in result. The following examples are for the purpose of *illustration only*, and should not be used to calculate unknowns. Each user should obtain their own standard curve.

**EXAMPLE ONE**

The following data was obtained for a standard curve using Calibrator Diluent I.

Standard (pg/mL)	O.D. (450 nm)	Mean	Zero Standard Subtracted (Std.) - (S1)
0	0.075, 0.063	0.069	0
62.5	0.109, 0.103	0.106	0.037
125	0.124, 0.152	0.138	0.069
250	0.288, 0.336	0.312	0.243
500	0.634, 0.747	0.691	0.621
1000	1.366, 1.484	1.425	1.356
2000	2.841, 2.955	2.898	2.829

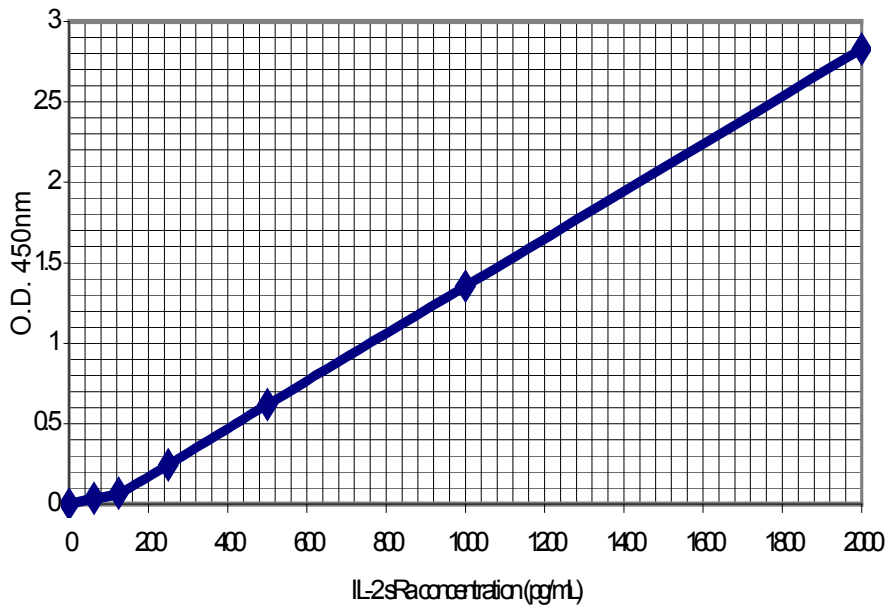


**EXAMPLE TWO**

The following data was obtained for a standard curve using Calibrator Diluent II.

Standard (pg/mL)	O.D. (450 nm)	Mean	Zero Standard Subtracted (Std.) - (S1)
0	0.102, 0.094	0.098	0
62.5	0.132, 0.122	0.127	0.029
125	0.178, 0.176	0.177	0.079
250	0.390, 0.349	0.369	0.271
500	0.755, 0.729	0.742	0.644

<b>1000</b>	<b>1.522, 1.504</b>	<b>1.513</b>	<b>1.415</b>
<b>2000</b>	<b>3.146, 3.315</b>	<b>3.231</b>	<b>3.133</b>

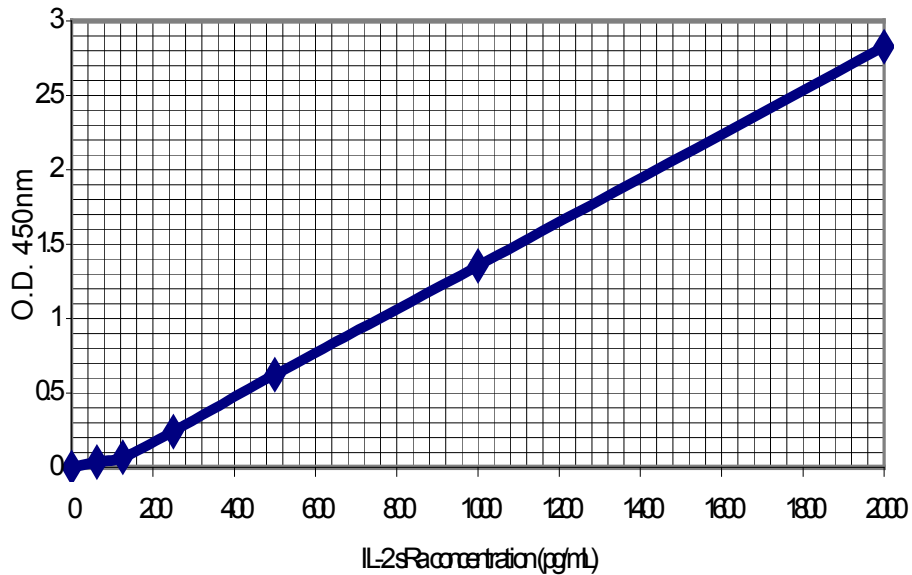

## PERFORMANCE CHARACTERISTICS

### 1. INTRA-ASSAY PRECISION

To determine within-run precision, three different samples of known concentration were assayed by replicates of twenty in 1 assay.

	<i>Calibrator Diluent I Assay</i>		
Sample	1	2	3
n	20	20	20
Mean (pg/ml)	158	426	431
Standard Deviation (pg/ml)	10.5	26.3	35.9
Coefficient of Variation (%)	6.6	6.1	8.3

	<i>Calibrator Diluent II Assay</i>		
Sample	1	2	3
n	20	20	20
Mean (pg/ml)	164	443	952
Standard Deviation (pg/ml)	9.8	29.5	39.2
Coefficient of Variation (%)	5.9	6.6	4.1

## 2. INTER-ASSAY PRECISION

To determine between-run precision, three different samples of known concentration were assayed by replicates on 20 different assays.

	<i>Calibrator Diluent I Assay</i>		
Sample	1	2	3
n	20	20	20
Mean (pg/ml)	160	451	925
Standard Deviation (pg/ml)	11.5	24.6	41.5
Coefficient of Variation (%)	7.1	5.5	4.5

	<i>Calibrator Diluent II Assay</i>		
Sample	1	2	3
n	20	20	20
Mean (pg/mL)	142	436	971
Standard Deviation (pg/ml)	9.8	24.2	39.9
Coefficient of Variation (%)	6.9	5.6	4.1

## 3. RECOVERY

By employing five random samples, the recovery of IL-2 sR $\alpha$  was evaluated in 7 varying amounts of IL-2 sR $\alpha$ . Throughout the range of the assay all samples were mixed and assayed in duplicate.

Sample Type	Average Recovery (%)	Range (%)
Cell Culture Media	104	95-115
Serum	105	100-118
EDTA plasma	104	93-110
Heparin plasma	104	95-111
Citrate plasma	105	92-116

## 4. SENSITIVITY

The minimum detectable quantity of human IL-2 sR $\alpha$  as observed by the standard curve generated for both Calibrator Diluent I and Calibrator Diluent II is 10 pg/mL. The two standard deviations above the mean optical density of the 20 replicates of the zero standard were defined as the minimum detectable quantities.

## 5. SPECIFICITY

This sandwich ELISA can detect both natural and recombinant human IL-2 sR $\alpha$ . This kit exhibits no significant cross-reactivity with factors related to or associated with IL-2 sR $\alpha$  such as rhIL-2, rhIL-2 sR $\alpha$ . No significant cross-reactivity was observed with recombinant human: IL-1 $\alpha$ , IL-1 $\beta$ , IL-1 sRI, IL-1 sRII, IL-1ra, IL-3, IL-3 sR $\alpha$ , IL-5, IL-5 sR $\alpha$ , IL-5 sRb, IL-6, IL-6 sR, IL-7, IL-8, IL-9, IL-10, IL-11, IL-12, IL-13 ANG, AR,

CNTF,  $\beta$ -ECGR, EGF, EPO, FGF acidic, FGF basic, FGF-4, FGF-5, FGF-6, FGF-7, G-CSF, GM-CSF, sgp 130, GRO  $\alpha$ , GRO $\beta$ , GRO $\gamma$ , HB-EGF, HGF, INF- $\gamma$ , IGF-I IGF-II, LAP (TGF- $\beta$ 1), LIF, M-CSF, MCP-1, MIP-1 $\alpha$ , MIP-1 $\beta$ ,  $\beta$ -NGF, OSN, PD-ECGF, PDGF-AA, PDGF-AB, PDGF-BB, PTN, RANTES, SCF, SLPI, TGF-  $\alpha$ , TGF- $\beta$ , TNF-  $\alpha$ , TNF- $\beta$ , sTNF RI, sTNF RII, VEGF.

#### 6. EXPECTED NORMAL VALUES

Biological samples from apparently healthy, normal individuals were collected and the average IL-2 sR $\alpha$  concentration measured. Serum samples (n=15) average value: 1265 pg/ml, range: 650-2216 pg/mL whereas plasma samples (n=15) average value: 1127 pg/ml, range: 540-3150 pg/mL.

#### REFERENCES

1. Chilosi, M., *et al.* (1987) Blood 70:1530.
2. Fernandez-Botran, R. (1991) FASEB J. 5: 2567.
3. Harrington, D.S., *et al.* (1988). Arch. Pathol. Lab Med. 112: 597.
4. Hatakeyama, M., *et al.* Science 244, 551-556.
5. Leonard, W.J., *et al.* (1994) Immunol Rev. 138: 61.
6. Leonard, W.J., *et al.* (1994) Curr. Opin. Immunol. 6: 631.
7. Minami, Y., *et al.* (1993). Annu. Rev. Immunol 11:245.
8. Pizzolo, G., *et al.* (1987) Br. J. Haematol. 67: 377.
9. Robb, R. J., *et al.* J. Exp. Med. 160, 1126-1146.
10. Rubin, L.A., *et al.* (1985) Hybridoma 4: 91.
11. Semenzato, G., *et al.* (1987) Blood 70: 396.
12. Sharon, M., *et al.* Science 234, 859-863.
13. Smith, K.A. (1989) Annu. Rev. Cell Biol. 5:397.
14. Steis, R.G., *et al.* (1988). Blood 71: 1304.
15. Takeshita, T., *et al.* J. Immunol. 148, 2154-2158.
16. Taniguchi, T and Y. Minami (1993) Cell 73: 5.
17. Teshigawara, K., *et al.* J. Exp. Med. 165, 223-238.
18. Tsudo, M., *et al.* Proc. Natl Acad. Sci. USA 83, 9694-9698.
19. Voss, S.D., *et al.* (1994) Blood 83: 626.
20. Wagner, D.K., *et al.* (1987) J. Clin. Oncol. 5:1262.
21. Waldmann, T.A. (1991) J. Biol. Chem. 266: 2681.
22. Waldmann, T.A. (1993) Immunol. Today 14: 264.
23. Wolf, R.E., *et al.* (1988) Arthritis Rheum. 31: 729.
24. Wang, H. M., *et al.* J. Exp. Med. 166, 1055-1069.